

Manual-PDD0100-5 1/9

# Six Transmitter Data communication Manual

If you are using our evaluation software "bioMON" this document is not relevant for you.



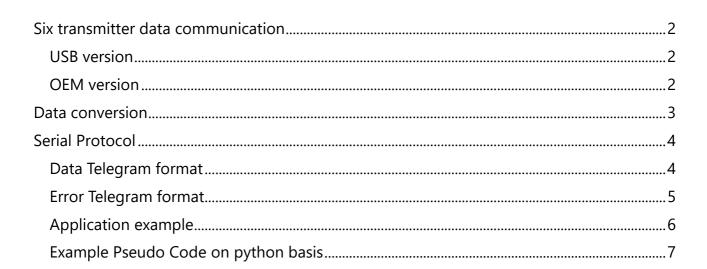

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

Manual-PDD0100-5 2/9

### Six transmitter data communication

You will have either the regular version with an USB cable or the OEM version without housing and cable.

#### **USB** version

#### **Win 10**

Follow these steps:

- 1. Assure you have Internet access.
- 2. Plug in the USB cable to the PC.
- 3. Download our evaluation software "bioMON": https://www.jobst-technologies.com/download/software/bioMON4\_Setup.zip
- 4. Install bioMON (this requires Admin privileges). Windows 10 will then automatically install a serial-to-USB driver for SIX.
- 5. You can keep bioMON installed, no matter if you will use it or not.

#### Win 7

Follow these steps:

- Download the serial-to-USB driver from: http://www.prolific.com.tw/US/ShowProduct.aspx?p\_id=225&pcid=41 that provides you a virtual COM port.
- 2. Plug in the USB cable to the PC.

#### **OEM** version

For the OEM version connect ground and supply voltage (3.3 – 5.5 V) to your power supply. Connect the Read data (Rx) pin of your microprocessor to the Send data (Tx) pin of the Six transmitter. The pin assignment can be found in the instrumentation datasheet *Biosensor Transmitter OEM*:

https://www.jobst-technologies.com/download/datasheets/instrumentation-datasheets/PDD0113-1\_Transmitter\_OEM\_datasheet\_en.pdf

There is no need to connect the Rx pin of the Six transmitter as the data is sent by the transmitter automatically every 1.7 seconds.

For the virtual serial port via USB interface or the TTL serial port (UART) with OEM version use port settings of 9600 baud, no parity, 8 data bits, and 1 stop bit (9600,n,8,1).

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

Manual-PDD0100-5 3/9

#### **Data conversion**

Having opened the port and powered up the Six transmitter it will send the data telegrams that you need to convert according to the following pages into the reading of the six sensor channels and the temperature.

You should have received factory calibration data from us as Definition text files like "216 1C.def". Its content shows like this (line numbers 1 – 7 added here for description):

- 3. -1,1,-1,1,1,18,0,17,17,17,17,17,17,18,0,0,0,0,0,0,0,0,0,0,0,0,0,0,0,0,0
- 4. "Blank1", "Glucose1", "Lactate1", "Blank 2", "Glucose 2", "Lactate 2", "Temperature"

#### Comments:

```
Line 1 holds the gain factors. Here: G_Blank1 = 0.1526, G_Glucose1 = 0.278, G_Lactate1 = 0.123, G_Blank2 = 0.1526, G_Glucose2 = 0.284, G_Lactate2 = 0.119
```

Line 4 holds the configuration of the chip you are using. In the example electrode 1 is **blank sensor**, etc.

Line 5 the channels to subtract. For chn1 none. For chn2 use chn1, etc.

Line 1 holds the actual calibration data. First entry 0.1526 converts chn1 readings into nA while the second entry is used to convert the difference of the AD counts of chn2-chn1 into mM of glucose, etc.

Line 7 holds the temperature sensitivity factors (e.g. **3.8** %/degC for chn2 = glucose 1) and the reference temperature (here **32** degC).

So using a 50nA range Six the concentrations in mM calculate as:

```
    Glucose_Signal_1 [mM] = (Chn2-Chn1) * G_Glucose1 / 100 / exp(0.038 * (Temperature - 32))
    Lactate_Signal_1 [mM] = (Chn3-Chn1) * G_Lactate1 / 100 / exp(0.032 * (Temperature - 32))
    Glucose_Signal_2 [mM] = (Chn5-Chn4) * G_Glucose2 / 100 / exp(0.038 * (Temperature - 32))
    Lactate_Signal_2 [mM] = (Chn6-Chn4) * G_Lactate2 / 100 / exp(0.032 * (Temperature - 32))
```

While using a 25nA range Six (info on range found on the backside label) use all (Gain factors/2) yielding:

```
• Glucose_Signal_1 [mM] = (Chn2-Chn1) * (G_Glucose1 / 2) / 100 / exp(0.038 * (Temperature – 32)) etc.
```

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

Manual-PDD0100-5 4/9

## **Serial Protocol**

## **Data Telegram format**

byte#	hex	Description	Comments
1.	68	Start	
2.	nn	Length	The length byte is the length from the number of data bytes + 1 (the message type id byte). Decimal value is 19.
3.	nn	Length	
4.	68	Start	
5.	04	Message type ID	Message type id is a unique number identifying the which message should be used to interpret the frame. Value is 4.
6.	XX	Channel1 Hi Byte	
7.	XX	Channel1 Lo Byte	
8.	XX	Channel2 Hi Byte	Frame data.
9.	XX	Channel2 Lo Byte	
10.	XX	Channel3 Hi Byte	If the value of one of the six channels is above 2^15 counts this represents a negative number.
11.	XX	Channel3 Lo Byte	Then subtract 2^16.  That gives a reading range of (-2^15) to +((2^15)-1) counts.  That range is equivalent to either +-25nA or +-50nA (check your Six transmitters label).  If the values are exactly 32767 or -32768 this indicates a value above/below the measurement boundaries i.e. an error.
12.	xx	Channel4 Hi Byte	
13.	XX	Channel4 Lo Byte	
14.	XX	Channel5 Hi Byte	
15.	XX	Channel5 Lo Byte	
16.	XX	Channel6 Hi Byte	
17.	xx	Channel6 Lo Byte	
18.	xx	Temperature Hi Byte	Divide the value by 16 to get the temperature in deg C.
19.	XX	Temperature Lo Byte	
20.	XX	ID Highest Byte (MSB)	
21.	XX	ID Byte 2	
22.	XX	ID Byte 3	
23.	xx	ID Lowest Byte (LSB)	
24.	XX	Checksum	The checksum is the last byte of sum of the values of the bytes of the message type id and the frame data (Bytes 5-23).
25.	16	Stop byte	

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

Manual-PDD0100-5 5/9

## **Error Telegram format**

1.	68	Start	
2.	nn	Length	The length byte is the length from the number of data bytes + 1 (the message type id byte). Decimal value is 2.
3.	nn	Length	
4.	68	Start	
5.	05	Message type ID	Value for Error message is 5.
6.	XX	Error code	
7.	xx	Checksum	The checksum is the last byte of sum of the values of the bytes of the message type id and the frame data (Bytes 5-6).
8.	16	Stop byte	

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

Manual-PDD0100-5 6/9

## **Application example**



For mM reading: Glucose\_Signal\_1 [mM] = (Chn2-Chn1) \* G\_Glucose1 / 100 / exp(0.038 \* (Temperature – 32))

For nA reading: Glucose\_Signal\_1 [nA] =  $(Chn2-Chn1) * G_Blank1 / 100 / exp(0.038 * (Temperature - 32))$ 

#G\_Blank1 is the blank gain factor provided in the .def file: G\_Blank1 = 50/((2^15)-1)\*100 = 0.1526

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

Manual-PDD0100-5 7/9

## **Example Pseudo Code on python basis**

The basic code example receives the byte array and gives the current in nA (for a 50 nA transmitter) per channel as well as the temperature and a timestamp

```
1. # -*- coding: utf-8 -*-
2. For Python3.7
@author: Jobst Technologies GmbH
5. This simple script reads data from a COM port, to which a SIX Potentiostat is
6. connected. Then it stores the timestamp in s, the current in nA and the temperature in de-
   gree C in a tab-delimited txt file.
7.
8. The SIX potentiotat delivers a data point every 1.7 seconds, which is shown on
9. screen and stored a tab-delimited txt file:
10. Timestamp in s
11. ch1 current in nA
12. ch2 current in nA
13. ch3 current in nA
14. ch4 current in nA15. ch5 current in nA
16.
      ch6 current in nA
17. Temperature in °C
19. Start conditions:
20. - SIX potentiostat is connected to a known COM port
21. - output file name
22. """
23. import serial
24. import time
25.
26. # Input data:
                                # This needs to be changed accordingly
27. COM PORT = "COM5"
28. OUT_FILENAME = "out_data.txt"
                                   # This needs to be changed accordingly
30. # Serial port settings
31. BAUD = 9600
32. TIMEOUT = 0.5
34. # Data telegram settings
35. package length = 25  # the SIX potentiostat delivers 25-bytes messages
36. data_block = [b'\x00'] * package_length # ring array for incomming data
37. start_timestamp = None
38.
39. # Starting serial port connection
40. with serial.Serial(COM_PORT, baudrate=BAUD, timeout=TIMEOUT) as ser, \
41. open(OUT_FILENAME, 'w') as file:
       # output first line
42.
43. first_line = "Time/s\tCh1/nA\tCh2/nA\tCh3/nA\tCh4/nA\tCh5/nA\tCh6/nA\tT/°C"
44.
      print(first_line)
45. file.write(first_line + "\n")
46. while(1): # Script will run until Ctrl+Z or Ctrl+C is pressed
      # Read data from serial port if available in the input buffer
47.
48.
49.
           if ser.inWaiting(): # is data in input buffer?
```

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

```
Manual-PDD0100-5
                                                                                               8/9
   50.
                   data = ser.read()
   51.
               if data is not None:
   52.
                    # operating with a ring array of size 25.
   53.
                   # data is inserted at 0 and removed at 25. Therefore,
   54.
                    # the data is inverted order in the array.
   55.
                   # array ==> [newest_byte .... oldest_byte]
                    # Each time the code parses the ring array is parsed until
   56.
   57.
                   # a valid telegram is recognized.
   58.
                    data_block.insert(0, data) # last byte in position 0
   59.
                   nirvana = data_block.pop()
   60.
                                                 # position 26 is deleted
                    del(nirvana)
                   header = [b' \times 04']
   61.
                                                 # Telegram header (inverted)
                              b'\x68',
   62.
                                                 # see documentation
                              b'\x13',
   63.
                              b'\x13'
   64.
                              b'\x68']
   65.
                   cks = 0 # checksum
   66.
   67.
                   # calculating checksum from byte 4 till second to last byte
   68.
                    for x in [int.from_bytes(x, 'big') for x in data_block[2:-4]]:
   69.
                        cks = (cks + x) & 0xFF
   70.
                    # validating header, end byte (x16) and checksum
   71.
                    if data block[-5:] == header \
   72.
                            and data block[0] == b'\x16' \
   73.
                            and int.from_bytes(data_block[1], 'big') == cks:
   74.
                        # now inverting data train
   75.
                       # Useful data are from byte 5 until second to last byte.
   76.
                        data_inv = [x for x in data_block[2:-5]]
   77.
                        data_inv.reverse()
   78.
                        it = iter(data_inv) # iterator used to fetch 2 bytes
   79.
                        # next line turns 2 bytes into a 16-bit integer array
   80.
                        out data = [
   81.
                            int.from_bytes(b''.join([x, next(it)]),
   82.
                                            byteorder='big',
   83.
                                            signed=True) for x in it]
   84.
                        # data to be stored
   85.
                       to_save = [str(x) for x in out_data] # 16-bit signed integers
                        # converting input data to currents in nanoamperes
   86.
   87.
                       # 50 nA ==> 32767 (2<sup>15</sup>-1)
   88.
                        # applying gain and updating data as nanoamp.
   89.
                        gain = 50 / (2**15 - 1)
   90.
                        to_insert = [str(round(int(x) * gain, 3)) for x in to_save[0:6]]
   91.
                        # converting temperature to °C
   92.
                        temperature = str(round(float(to_save[6]) / 16, 3))
   93.
                        to insert.append(temperature)
   94.
                        # generating timestamps
   95.
                       timestamp = round(time.time(), 4)
   96.
                        if start timestamp is None:
   97.
                            start timestamp = timestamp
   98.
                            delta_time = 0
   99.
                        else:
                             delta_time = timestamp - start_timestamp
   100.
   101.
                         to_insert.insert(0, str(round(delta_time, 1)))
   102.
                         # printing data on screen and output file
                         print("\t".join(to_insert))
   103.
   104.
                         file.write("\t".join(to_insert) + "\n")
   105.
                         # Next data point arrives in about 1.6 seconds
   106.
                         # So, resting for 1.4 seconds should be enough
```

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520

Manual-PDD0100-5 9/9

107. time.sleep(1.4)
108. time.sleep(0.01) # Default polling time

Disclaimer: Evaluation product for professionals to be used solely for research and development purposes! Not for medical and diagnostic use. Not to be used on humans. For more information contact IST AG.

Fon: +49 761 5577520